


Hamilton C1 Ventilator




Press and then confirm to pause ventilation

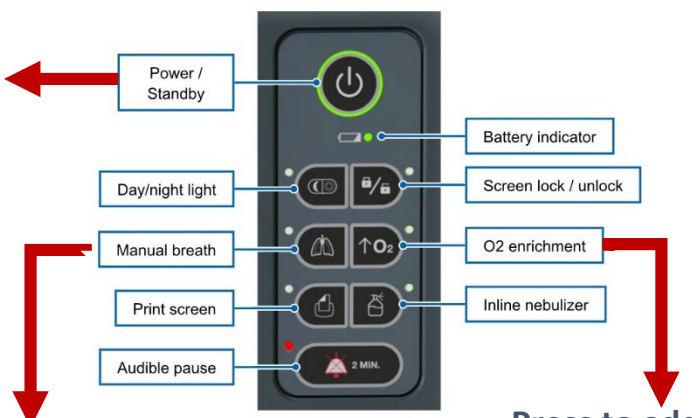

Press and hold to perform inspiratory pause


Press to add 100% FiO₂ to inspiratory circuit

How to change settings? Touch screen and turn knob

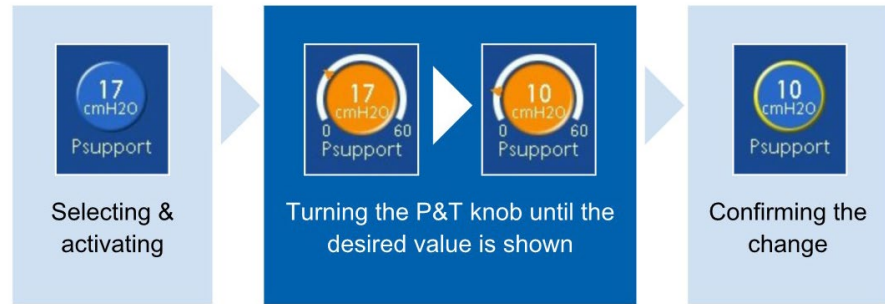

Touch to change ventilator mode

Displays Alarm Message

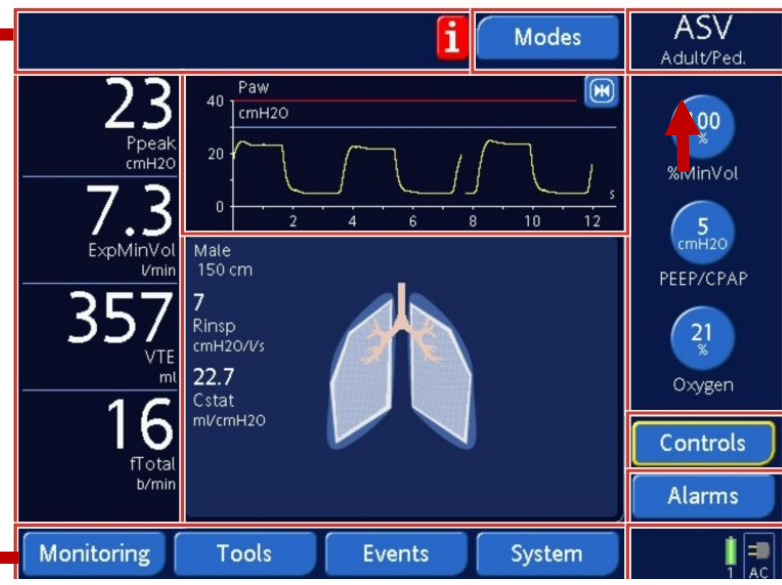

Touch to change ventilator settings

Touch to change alarm limits

Touch to view patient mechanics data

