


Intraoperative Biomechanics of Lumbar Pedicle Screw Loosening Following Successful Arthrodesis

Hope B. Pearson,¹ Christopher J. Dobbs,² Eric Grantham,² Glen L. Niebur,¹ James L. Chappuis,² Joel D. Boerckel ^{1,3}

¹Department of Aerospace and Mechanical Engineering, University of Notre Dame, 142 Multidisciplinary Research Building, Notre Dame, Indiana 46557, ²Spine Center Atlanta, 3161 Howell Mill Road Suite 400, Atlanta, Georgia 30327, ³Departments of Orthopaedic Surgery and Bioengineering, University of Pennsylvania, Claire M. Fagin Hall, 418 Curie Blvd, Philadelphia, Pennsylvania 19104

Received 29 September 2016; accepted 28 March 2017

Published online 11 July 2017 in Wiley Online Library (wileyonlinelibrary.com). DOI 10.1002/jor.23575

ABSTRACT: Pedicle screw loosening has been implicated in recurrent back pain after lumbar spinal fusion, but the degree of loosening has not been systematically quantified in patients. Instrumentation removal is an option for patients with successful arthrodesis, but remains controversial. Here, we quantified pedicle screw loosening by measuring screw insertion and/or removal torque at high statistical power ($\beta = 0.02$) in $N = 108$ patients who experienced pain recurrence despite successful fusion after posterior instrumented lumbar fusion with anterior lumbar interbody fusion (L2–S1). Between implantation and removal, pedicle screw torque was reduced by 58%, indicating significant loosening over time. Loosening was greater in screws with evoked EMG threshold under 11 mA, indicative of screw misplacement. A theoretical stress analysis revealed increased local stresses at the screw interface in pedicles with decreased difference in pedicle thickness and screw diameter. Loosening was greatest in vertebrae at the extremities of the fused segments, but was significantly lower in segments with one level of fusion than in those with two or more. Clinical significance: These data indicate that pedicle screws can loosen significantly in patients with recurrent back pain and warrant further research into methods to reduce the incidence of screw loosening and to understand the risks and potential benefits of instrumentation removal. © 2017 Orthopaedic Research Society. Published by Wiley Periodicals, Inc. *J Orthop Res* 35:2673–2681, 2017.

Keywords: biomechanics; pedicle screw; lumbar spinal fusion; loosening

Chronic low back pain is the second most-common reason for visits to a physician in the United States, and interbody fusion is common in patients non-responsive to non-surgical options.¹ In 2012, over 413,000 lumbar fusions were reported in the United States, and demand for surgical treatment continues to rise.^{2,3} Improvements in surgical approaches,⁴ as well as fixation instrumentation^{4,5} and inductive bone formation agents^{2,6,7} have improved patient outcomes, reduced the frequency and extent of complications, and have collectively made lumbar spinal fusion a common procedure that has improved quality of life for millions of patients.

However, reoperation secondary to recurrent back pain has been reported in approximately 14–27% of patients,⁸ with complications including improper instrumentation placement, loss of fixation, fatigue and bending failure, dural tears, nerve root injury, infection, and pedicle screw loosening.^{9,10} While successful fusion is correlated with desirable clinical outcomes,¹¹ recurrent pain can occur even in patients with solid arthrodesis, which may be associated with instrumentation loosening, requiring revision, or removal.

Over the past 10 years, posterior pedicle screw systems have increased in strength and rigidity,^{12,13} increasing pre-fusion stability and decreasing the inci-

dence of pseudarthrosis.^{13,14} However, this has also increased the loads present at the bone-screw interface due to increased load-sharing,¹⁵ which may contribute to pedicle screw loosening.^{16,17} In addition, moderate load sharing under compliant fixation stimulates bone formation, but excessive motion induces pseudoarthrosis,¹⁷ potentially through the inhibition of neovascularization.¹⁸ Surgical removal of pedicle screws has been much discussed,^{10,19} and remains controversial due to the associated risks of secondary surgery and potential for instability following removal.²⁰ However, when unexplainable recurrent pain is severe, screw removal has been recommended,^{21–24} and may also reduce risks of metal toxicity and hypersensitivity.²⁵

We hypothesized that patients with recurrent pain, despite successful arthrodesis, would exhibit pedicle screw loosening. Therefore, the aims of this study were to quantify pedicle screw loosening in patients with recurrent back pain following successful posterior instrumented lumbar fusion (PILF) surgery and to assess patient pain perception prior to and following instrumentation removal.

METHODS

This is a retrospective cohort study with level of evidence of Level II.

Patients

A total of 108 patients (75 male, 33 female), 29–78 years of age (mean 47, SD 11), were voluntarily enrolled following exclusion criteria according to STROBE (strengthening the reporting of observational studies in epidemiology) guidelines (Fig. 1A). A single surgeon (JLC) performed all procedures. Each patient had been diagnosed with degenerative spinal stenosis with associated instability, degenerative spondylolisthesis, or annular tears and discogenic pain that had failed

Conflicts of interest: None.

Grant sponsor: Indiana CTSI; Grant number: NIH/NCRRL1TR001108.

Correspondence to: James L. Chappuis and Joel D. Boerckel (T: 404-879-5091 (JLC), 574-631-1866 (JDB); F: 404-351-6017 (JLC), 574-631-2144 (JDB); E-mail: jchappuis@spineatl.com (JLC), jboercke@nd.edu (JDB))

© 2017 Orthopaedic Research Society. Published by Wiley Periodicals, Inc.

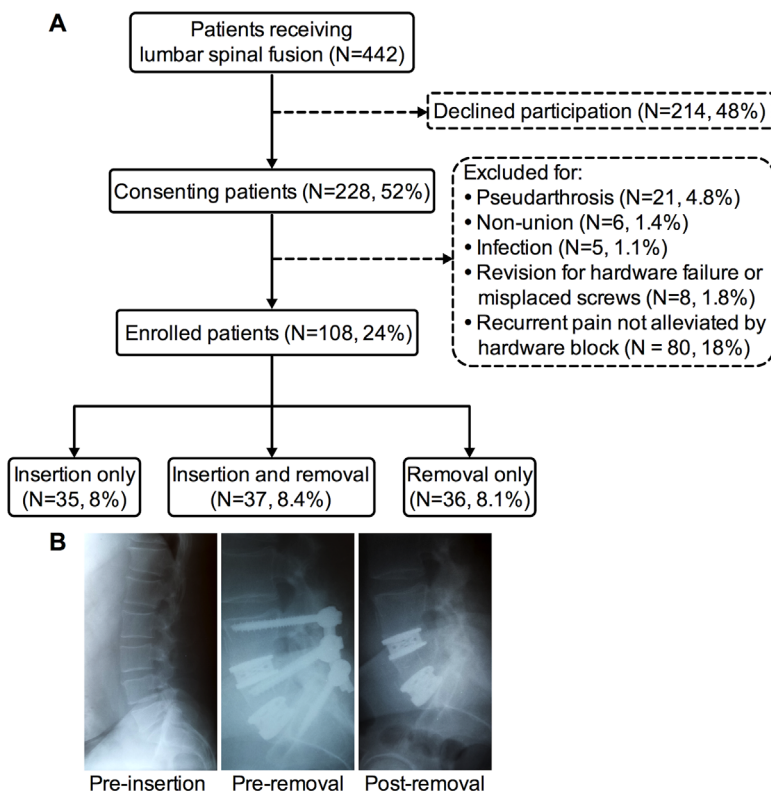


Figure 1. Patient selection and pedicle screw removal. (A) STROBE flowchart of subject inclusion and exclusion. (B) Representative X-ray images of pedicle screw removal following successful arthrodesis at pre-insertion, post-fusion, and post-removal time points.

conservative treatment for at least 1 year. All subjects gave informed consent to participate, and the study was approved by Sterling Institutional Review Board, Atlanta, GA (#5187). Patients received 2- to 5-level spinal fusion of lumbar vertebrae between L2 and S1 (Fig. 1B).

Only patients with successful arthrodesis were selected for subsequent evaluation. Patients who returned with complaints of recurrent pain that could not be explained by alternative diagnoses such as insufficient fusion or pseudarthrosis, infection, instrumentation failure, or soft tissue injury, and who elected both instrumentation removal and informed inclusion in the study were selected for analysis. To verify that recurrent pain was instrumentation-associated, anterior and posteriolateral computed tomography (CT) scans were assessed to rule out pseudarthrosis, adjacent segment disease, and sagittal imbalance. Further, following a radiopaque dye injection (10 cc Amipaque) under C-arm guidance to provide X-ray contrast, a peri-implant “hardware block” was performed by Marcaine injection (1%, 20 cc), and ambulatory patient pain was evaluated. Only patients with successful arthrodesis whose pain could be attributed to the instrumentation by hardware block were then selected for instrumentation removal in a second surgery. Measurements at both insertion and removal were taken in 37 patients (12 male, 25 female) for paired assessment. Measurements at insertion only were assessed in 35 patients (32 male, 3 female), and measurements at removal only were taken in 36 patients (31 male, 5 female). Removal torque measurement was assessed at an average \pm SD of 266 ± 73 days post-implantation.

Surgical Approach

Patients received posterior instrumented lumbar fusion (PILF) combined with anterior lumbar interbody fusion (ALIF) to maximize segment stability (Fig. 1B). Briefly, patients were placed prone on a Jackson operating table,

prepped, and draped in usual sterile fashion. After open exposure of the pedicles, pedicle holes were tapped and titanium pedicle screws (TSRH-3D[®]) were inserted under C-arm guidance based on the standard progression of coronal angle (5° at L1, progressing 5° at each successive caudal level). In the sagittal plane, screws were inserted level with the pedicle and disc space without caudal/cephalad angling. Screw diameters were chosen according to manufacturer's recommendations, and lengths were selected to achieve 60–80% engagement in the vertebral body upon full insertion. Holes were tapped 1 mm diameter smaller than the screw size (i.e., undertapped), yielding a screw-hole interference fit, $\delta_i = r_s - r_h = 0.5$ mm, where r_s is the radius of the pedicle screw, and r_h is the radius of the tapped hole prior to screw insertion.²⁶

The decision to proceed with instrumentation removal in consenting patients was made upon verification of successful arthrodesis by computed tomography scan in both anterior and posterolateral views and nullification of alternative explanations. A total of 80 patients with recurrent pain did not receive hardware removal due to inability to identify the hardware as cause of recurrent pain (Fig. 1A). Selected patients were returned to the operating room no sooner than 6 months after insertion and up to 3 years (mean \pm SD 266 ± 73 days) after the initial procedure. Instrumentation was exposed in routine fashion, and side connectors and rods were removed. Screw complications were not observed prior to removal. Beam-hardening artifacts limited our ability to assess peri-implant radiodensity by computed tomography on post-implantation and pre-removal scans.

Pedicle Screw Insertion and Removal Torque

Pedicle screw insertion ($N=467$) and removal ($N=477$) torques were measured using a sterilizeable, manual

mechanical torque wrench (Mountz, San Jose, CA), with $N=139$ paired insertion and removal measurements in the same patients. To ensure changes in torque between insertion and removal surgeries did not occur due to hole tapping by the insertion screw, pedicle screw back-out torque (at the time of insertion) was also measured ($N=204$).

Evoked EMG Stimulus Threshold

Paired evoked electromyographic (EMG) stimulus thresholds through the screw hole²⁷ were measured in $N=98$ screws. Non-paired measurements at insertion ($N=394$) and removal ($N=430$) were also taken.

Screw and Pedicle Measurements

Vertebral level, screw type, diameter, and length were recorded for each inserted or removed screw. Pedicle thickness was measured from pre-insertion digital CT scans in the transverse plane, and pedicle-screw diameter difference, defined as pedicle thickness minus screw diameter was computed.²⁸

Stress Analysis

A theoretical stress analysis of monotonic cantilever loading in transverse compression and bending and press-fit by screw insertion was performed to estimate the stresses in peri-implant pedicle bone with or without loosening of the screw. The trabecular bone of the pedicle was assumed to have an effective modulus of 42.8 MPa and a Poisson ratio of 0.25, while the cortical bone was assigned a modulus of 21 GPa and a Poisson ratio of 0.37 (Appendix Table SA1).^{29–32} The modulus of the titanium screws was assumed to be 180 MPa. Loading of the spine causes cantilevered loads and moments to be transmitted through the instrumentation, resulting in both a transverse load and moment to be distributed to the surrounding trabecular bone along the embedded length of the screw. The stresses induced by this cantilever loading can be approximated by beam-on-elastic-foundation theory,³² assuming the screw and cortical bone act as co-axial deformable beams joined by an elastic foundation of trabecular bone, assumed here to be homogeneous. See Appendix S1 for the associated differential equations, boundary conditions, and solution approach. We evaluated the stress distribution in the trabecular bone along the length of the pedicle screw and computed the maximal stress, $\sigma_{r_{cantilever}}$, which occurred at the screw insertion point ($z=L$; labeled as point A in Fig. 6A). Since the flexural rigidity of the trabecular bone is substantially lower than either the cortical bone or titanium screw, the axial stresses in the elastic trabecular layer due to bending can be neglected. Local stresses were assessed under physiologic loading conditions of standing, extension, and flexion,^{33,34} with assumptions of either loosened or bonded screws, as described in Appendix S1.³² Next, a press-fit analysis based on linear elastic thick-walled pressure vessel theory was used to determine the “locked-in” stress induced by the insertion of the screw for the given screw-hole interference fit ($\delta_i=0.5$ mm). See Appendix S2 for associated differential equations, boundary conditions, and solution approach. To determine the composite stress state as a superposition of the residual stresses from the combined cantilevered loading and interference fit, the maximum von Mises stress in the pedicle at the screw

interface, σ_H , was defined as:

$$\sigma_H = \frac{1}{\sqrt{2}} \left[(\sigma_1 - \sigma_2)^2 + (\sigma_2 - \sigma_3)^2 + (\sigma_3 - \sigma_1)^2 \right]^{\frac{1}{2}} \quad (1)$$

where $\sigma_1 = \sigma_{r_{interference}} + \sigma_{r_{cantilever}}$, $\sigma_2 = \sigma_{\theta_{interference}}$, and $\sigma_3 \approx 0$.

Visual Analog Scale Assessment of Patient Pain

Finally, to evaluate patient perception of lumbar pain, patients ($N=31$ complete responders) were self-assessed using the visual analog scale (VAS; 0–100 mm) prior to fusion surgery, 1 month after insertion, prior to removal, 0–3 months after removal, and 3–6 months after removal. Self-reporting of the degree of analgesic medicine use and activity were also assessed using the same VAS approach.

Statistical Analysis

Differences between groups were evaluated by two-tailed Student's *t*-test or analysis of variance (ANOVA) followed by Tukey's post-hoc test for single and multiple comparisons, respectively, when assumptions of normality and homoscedasticity were met by D'Agostino-Pearson omnibus normality and *F*-tests, respectively. Otherwise, non-parametric Mann-Whitney and Kruskal-Wallis followed by Dunn's multiple comparison tests were used. The *p*-values less than 0.05 were considered significant. For paired measurements, differences were analyzed by paired Student's *t*-test or Wilcoxon's matched-pairs signed rank test. Correlations between groups were assessed by linear regression using Pearson's coefficient of determination (R^2).

RESULTS

Insertion and Removal Torque

Paired insertion and removal torque measurements ($N=139$ pairs) revealed a significant 58.1% lower removal torque compared to insertion of those same screws ($p<0.0001$), with only 9% of screws loosening by less than 15% (Fig. 2A). To ensure that this reduction in torque between insertion and removal was not simply due to tapping of the screw hole during insertion of the screw, the single-rotation back-out torque was also evaluated at the time of insertion. The immediate torque loss between insertion and back-out was $1.4 \pm 5.6\%$ (Fig. 2B; $p=0.68$, $\beta < 0.02$). Samples were clustered at a mean percent change of 0% (Fig. 2B, right). Non-paired insertion ($N=467$) and removal torques ($N=477$) were also evaluated to determine whether a similar difference in torque would also be apparent in non-paired samples, and revealed a similar 68% difference in torque between insertion and removal ($p<0.0001$, Supplemental Fig. S1A).

Loosening by Vertebral Level

The percent torque loss by vertebral level in paired samples was evaluated at five levels of vertebrae from L2 to S1 (Fig. 3A; pairings showing adjacent segments within the same patient illustrated by connecting lines). The greatest degree of loosening was observed in L2 and S1, and the least in L4 ($p<0.05$ by ANOVA with Tukey's post-hoc test). To determine whether this

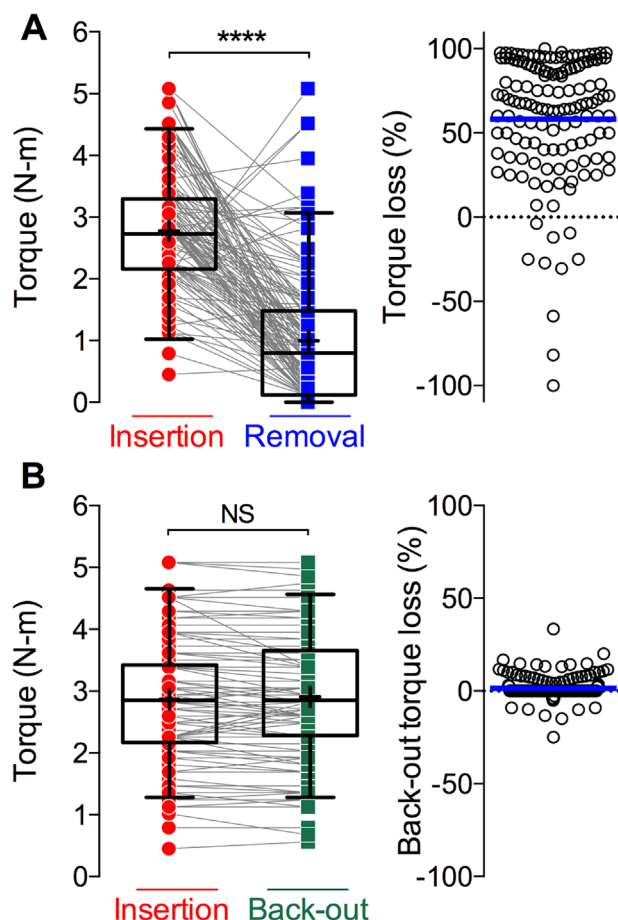


Figure 2. Measurement of pedicle screw loosening by insertion and removal torque. (A) Insertion and removal torque with paired samples connected by gray lines ($N=139$ pairs), and scattergram of percent torque loss for those same pairs. (B) Insertion and immediate back-out torque ($N=204$ pairs). Box plots show median line and 25th, and 75th percentiles, with whiskers at 5th and 95th percentiles, respectively. Mean values indicated by + symbol. Scattergrams show mean values indicated by blue line. Statistical differences assessed by paired two-tailed Student's t -test. **** $p < 0.0001$; NS, not significant.

was inherent to the vertebral level or whether the fused segments at the ends of the fusion exhibit more loosening, we compared the torque loss in the superior and inferior extremes of the fused segments versus internal segments, and found greater loosening in vertebrae at the edges of the fusion segment ($p < 0.05$; Fig. 3B). No differences were found between the superior-most versus inferior-most segments. Next, we evaluated the mean torque loss as a function of the number of fused vertebrae (Fig. 3C). While all levels exhibited significant loosening, screws from segments with a single level of fusion exhibited measurably less loosening compared to those with multiple levels of fusion ($p < 0.05$). Similar trends were observed for non-paired samples (Supplemental Fig. S2).

Evoked EMG Stimulus Threshold

A difference in stimulus threshold at the screw hole was not measurable between insertion and removal ($p > 0.05$, $\beta = 0.11$; Fig. 4A). However, torque loss in

samples with less than 11 mA threshold at insertion, which has been identified as an indicator of screw placement and pedicle cortex violation,²⁷ was significantly greater than those with insertion threshold above 11 mA ($p < 0.05$, Fig. 4B). For unpaired measurements, the stimulus threshold at screw removal was 15% lower than the stimulus threshold at insertion ($p < 0.0001$, $N = 427, 393$, respectively; Supplemental Fig. S1B).

Correlation Analysis

Correlation analyses were performed to determine whether insertion torque, screw geometry, pedicle-screw diameter difference, or EMG stimulus threshold in the pedicle could predict loosening. Insertion torque correlated with torque loss ($p < 0.01$), but with little predictive power ($R^2 = 6\%$; Fig. 5A). Neither screw diameter nor length³⁵ predicted the extent of torque loss, even in long screws with increased vertebral body penetration (Fig. 5B,C). Torque loss was weakly correlated with little predictive power ($p = 0.14$, $R^2 = 3\%$) with pedicle screw-diameter difference as a measure of geometric pedicle integrity post-insertion (Fig. 5D). EMG stimulus threshold did not linearly correlate with loosening either at insertion or at removal (Supplemental Fig. S3).

Stress Analysis

Analytical models were used to estimate the stress distribution in the peri-implant bone along the length of the screw for cantilevered screw loads and moments using reported values for physiologic static loading conditions under standing, extension, and flexion poses^{33,34} (Fig. 6A,C). Screw-hole interference stresses were calculated to approximate the press-fit-induced radial and circumferential stresses in the trabecular and cortical bone as a function of radial position (Fig. 6B,D). The location of maximal von Mises stress occurred at the insertion point, immediately adjacent to the screw (indicated by Point A in Fig. 6A,B). Under the applied loading conditions, the local von Mises stress decreased with increasing pedicle-screw diameter difference, shown overlaid with measured torque loss (Fig. 6E). The degree of pedicle-screw diameter difference substantially influenced local stress values.

Patient Pain Perception

While pain perception in these patients was significantly reduced by 19% within 1 month after surgery, pain was recurrent, and returned to 89% of pre-surgery levels, causing patients to return for instrumentation removal surgery (Fig. 7). Following removal, mean VAS pain scores returned to post-insertion levels, but differences with pre-removal pain were not statistically significant. From 3 to 2 months after removal surgery, mean VAS pain scores remained at 27% lower than the pre-insertion levels. No differences were found in patient-reported use of

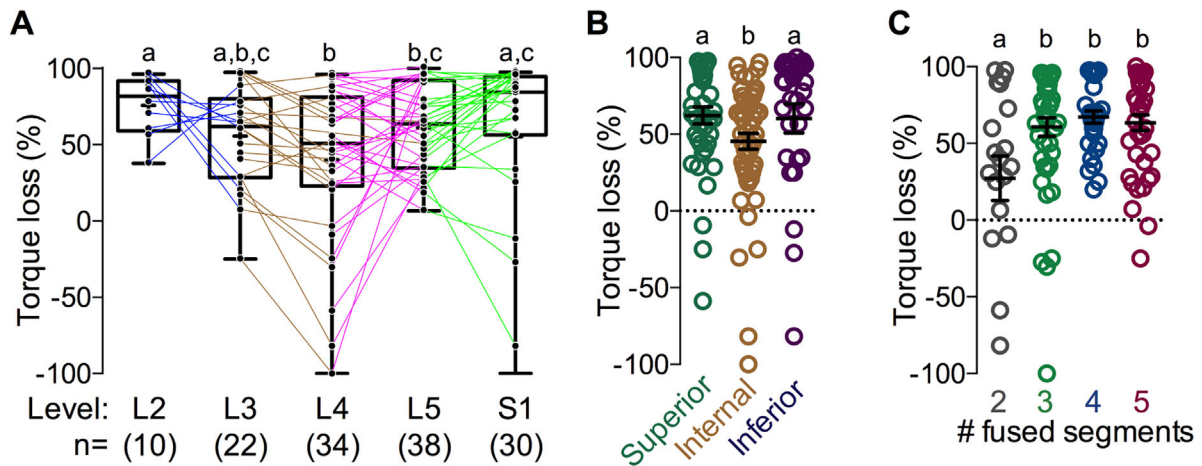


Figure 3. Pedicle screw loosening by vertebral level. (A) Percent torque loss for vertebral levels L2–S1 for paired measurements ($N=139$). Box plots show median line and 25th, and 75th percentiles, with whiskers at 5th and 95th percentiles, respectively. Mean values indicated by + symbol. (B) Torque loss in internal segments versus those at the extremes of the fusion segment (superior/inferior), shown with mean \pm s.e.m. (C) Torque loss as a function of number of levels of fusion, shown with mean \pm s.e.m. Significance indicator letters shared in common between groups indicate no significant difference in pairwise comparisons ($p > 0.05$).

analgesics or physical activity between any time points (Supplemental Fig. S4).

DISCUSSION

Taken together, these data indicate that pedicle screws can loosen over time by an average of 58%, even after successful arthrodesis, in patients with recurrent back pain. This is significant because, while screw loosening on removal has been observed previously in a small pilot study,³⁶ this is the first demonstration of the prevalence and degree of this problem. Sandén et al.³⁶ evaluated pedicle screw loosening in eight patients, observing a 61% reduction in torque, which is highly consistent with our observations. They found that insertion torque correlated with

removal torque in six screws, but the remaining measurements exhibited no discernable correlation. Consistent with this observation, our data suggest that only 6% of the variation in loosening can be predicted by insertion torque. Additionally, our data implicate screw placement, pedicle-screw diameter difference, fusion level, and number of fused vertebrae as important biomechanical factors in screw loosening.

Certainly, measures that could predict loosening a priori would have significant clinical utility, though this is challenging due to the multifactorial nature of screw loosening. Other studies have also evaluated insertion torque as a potential predictor, with some proposing this measure as a better predictor than bone mineral density,^{37–39} but its correlation with linear pullout strength in cadaveric studies is weak ($R^2=0.04$ – 0.4).^{40,41} Consistent with these observations, we found that insertion torque correlated significantly with torque loss, but the predictive power was poor ($R^2=6\%$ for $N=139$ pairs), indicating that intraoperative measurement of pedicle screw insertion torque is not uniquely sufficient to predict the degree of loosening.

Evoked EMG stimulus threshold is frequently used to detect screw placement and pedicle cortex violation, and could also be indicative of osteopenia.^{27,42} In the present study, intraoperative EMG measurements indicated that screws with EMG thresholds less than 11 mA, indicative of poorly seated screws or screws in osteopenic bone, have a greater likelihood of loosening; however, EMG stimulus threshold could not linearly predict the degree of loosening. These observations suggest that further research is warranted to decouple the interactions between local mineral density, screw placement and angle, and pedicle screw loosening. The evoked EMG stimulus threshold is commonly used to assess pedicle wall violation and nerve root exposure,²⁷ so screw loosening may therefore induce late-onset

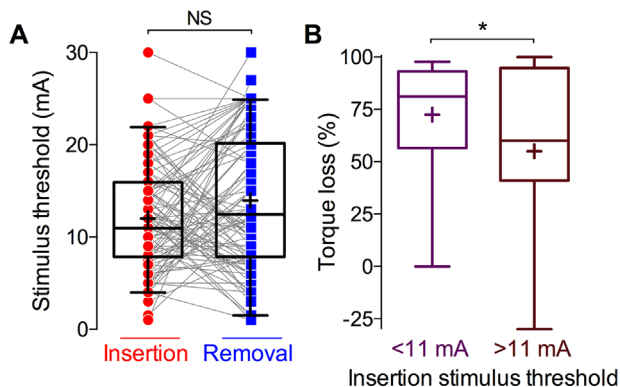


Figure 4. Evoked EMG stimulus threshold at insertion and removal. (A) Insertion and removal stimulus threshold with paired samples connected by gray lines ($N=98$ pairs). (B) Percent torque loss for paired samples with insertion stimulus threshold less than (purple) or greater than (brown) the 11 mA cutoff indicative of pedicle screw placement quality.²⁷ Box plots show median line and 25th, and 75th percentiles, with whiskers at 5th and 95th percentiles, respectively. Mean values indicated by + symbol. Statistical differences assessed by paired (A) and unpaired (B) two-tailed Student's t -test. * $p < 0.05$; NS, not significant.

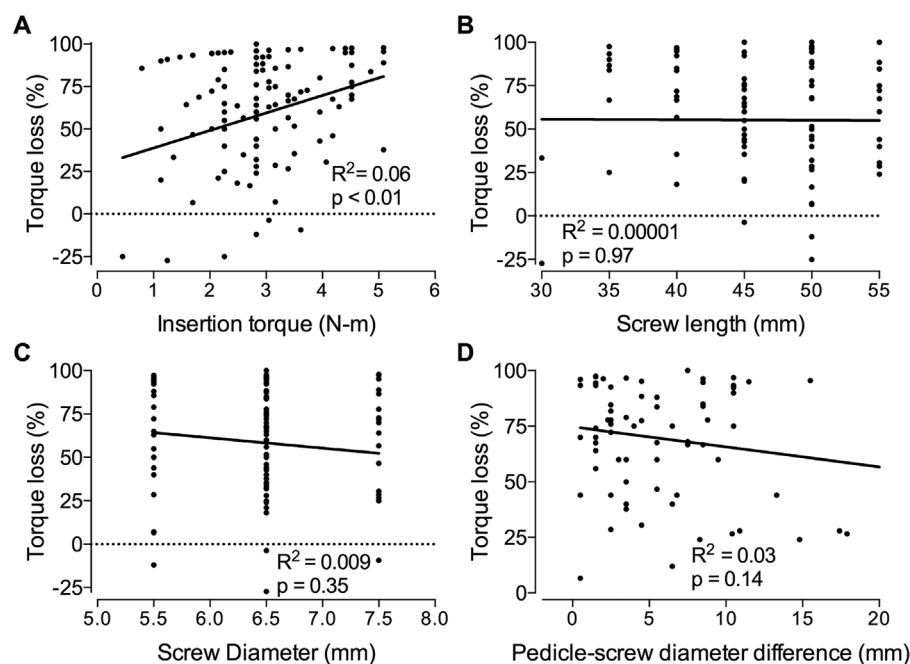


Figure 5. Linear regression analysis of pedicle screw loosening for intraoperative measurements. Correlation of percent torque loss with: (A) Insertion torque ($N = 139$), (B) screw length ($N = 114$), (C) screw diameter ($N = 139$), (D) pedicle-screw diameter difference ($N = 106$).

nociceptive pain through stimulation of mechanosensitive nerve fibers upon progressive degradation of the peri-implant bone matrix.

The degree of loosening was vertebral level-dependent in a biphasic manner, with the least amount of loosening in the middle of the range of operated segments, and increased loosening in vertebrae at the extremities of the fused segments; however, screws in patients with a single level of fusion exhibited measurably lower torque loss than those with fusion of three or more vertebrae. Together, these data implicate biomechanical stability as an important factor in pedicle screw loosening.

The mechanisms that contribute to pedicle screw loosening are certain to be multifactorial, with both mechanical and biological components. One possibility is instrumentation-induced stress shielding and subsequent disuse osteopenia. A decrease in bone mineral density under stiff fixation has been seen in both canine^{43,44} and human⁴⁵ implanted fixation devices as a result of stress shielding. Conversely, transfer of moderate levels of mechanical stimuli through compliant fixation can enhance BMP-2-induced bone formation in large defects, though excessive motion can induce pseudarthrosis and non-union.^{17,18,46} Thus, the optimal rigidity of spinal fixation instrumentation remains a subject of ongoing investigation. Another likely contributor is local plastic deformation at the bone-screw interface caused by the insertion and cyclic loading of the pedicle screws, resulting in screw toggling and loosening. Pedicle screw insertion also induces residual stresses and stress concentrations that superimpose with cyclic loads to contribute

to local tissue failure. These stresses are highest at the cap-rod-screw interface,^{47,48} as we demonstrate using beams-on-elastic-foundation and thick-wall pressure vessel theory. Reported yield stresses for spinal trabecular bone range from 3 to 96 MPa.^{49,50} Using the von Mises stress as a measure of failure propensity, we calculated local stresses at the screw entry point of 50 MPa at median pedicle/instrumentation geometries, suggesting that local stresses may contribute to loosening through load-induced toggling. These values are consistent with prior reports of static vertebral von Mises stresses up to 100 MPa at the pedicle body junction. Incorporation of pedicle screw loosening into the model revealed increased stresses at the screw insertion point following screw loosening, which would positively feed back to promote further loosening consistent with a prior finite element comparisons of stresses around loosened and bonded pedicle screws.⁴⁷ A recent hybrid multibody/finite element study by Fradet et al.⁵⁰ evaluated the stresses induced by simulated intraoperative scoliosis correction maneuvers as well as failure loading of the instrumented spine, without fusion. They identified surgical maneuvers induced stresses of 40–100 MPa at the screw entry point.⁵⁰ Notably, their model, which featured L1–L3 fusion, identified maximal screw interface stresses in the proximal-most segment, L1, consistent with the loosening trends observed here. Together, these data suggest that both biological and mechanical factors influence the etiology of pedicle screw loosening, and further research is needed to elucidate the mechanisms underlying the initiation and progression of screw loosening as well as clinical

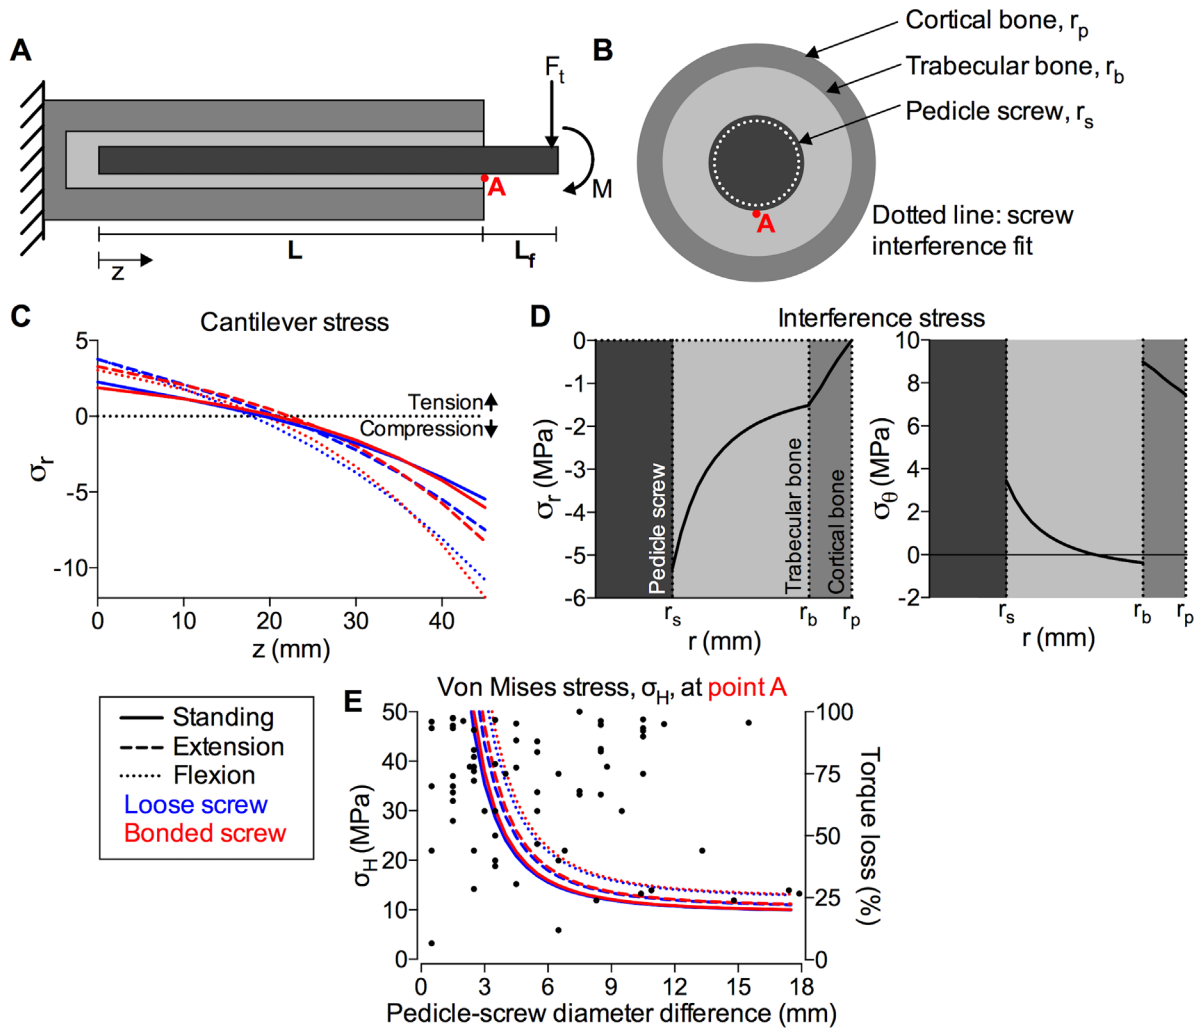


Figure 6. Analysis of stresses induced by cantilevered instrumentation loading and screw interference fit. (A) Schematic of the screw and pedicle approximated as co-axial beams joined by an elastic foundation of trabecular bone with a cantilever load applied to the screw resulting in a transverse load, F_t , and a moment, M . (B) Schematic of interference fit. (C) Stress distribution along the screw under physiologic loading conditions for standing, extension, and flexion of the spine assuming either the screw is either loose (blue) or perfectly bonded (red). (D) Radial and circumferential stresses induced by screw insertion assuming an interference fit of $\delta_i = r_s - r_h = 0.5$ mm. (E) Von Mises stress at the location of maximal stress (labeled point A) as a function of pedicle-screw diameter difference superimposed on percent torque loss as measured in patients.

implications for surgical approach and post-operative pain management.

This model did not account for bone remodeling induced by local damage or biological responses to the implant, which can also change and progress over time.⁵¹ High static stresses, combined with cyclic fatigue loading, may drive local pedicle failure and cause loosening over time. Screw trajectory also influences the biomechanical environment⁵² and its impact on loosening requires further research. Our observations together suggest that increasing screw size relative to either pedicle thickness or initial hole diameter may impair long-term stability as a result of local stress concentration. Future studies will be required to evaluate whether patients with low pedicle thickness exhibit increased likelihood of loosening, requiring additional observation or screw augmentation.

While the full clinical implications of pedicle screw loosening in balance with the potential negative sequelae of spinal instrumentation removal will require further study, these data suggest that pedicle screw loosening is prevalent in patients with recurrent pain, despite successful arthrodesis. This study was unable to determine whether screw loosening is present in patients without recurrent pain since unwarranted instrumentation removal for purely observational purposes would not be in the best interests of the patients. However, our observations of patient pain perception are in agreement with several studies, suggesting that pedicle instrumentation removal following successful arthrodesis may relieve recurrent pain,^{21–24} potentially caused by pedicle screw loosening. Further research will be necessary to fully evaluate clinical and pain outcomes and to establish pedicle screw loosening as a causative factor.

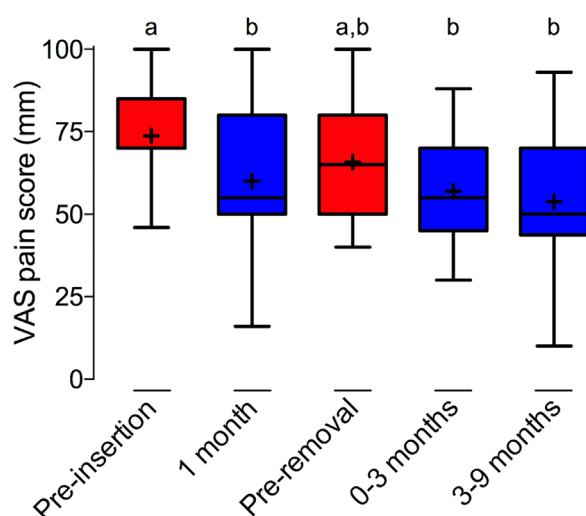


Figure 7. Patient assessment of recurrent pain. Visual Analog Scale (VAS; 0–100 mm) assessment of pain ($N=31$). Box plots show median line and 25th, and 75th percentiles, with whiskers at 5th and 95th percentiles, respectively. Mean values indicated by + symbol. Significance indicator letters shared in common indicate no significant difference in pairwise comparisons ($p > 0.05$).

AUTHORS' CONTRIBUTIONS

JLC performed surgeries; HBP, CJD, EG collected data; HBP, GLN, JDB performed data analysis; HBP, JLC, and JDB wrote the paper; all authors read and approved the final submitted manuscript.

ACKNOWLEDGMENTS

We gratefully acknowledge funding (to JDB) from the Indiana Clinical and Translational Sciences Institute funded, in part by Grant Number UL1TR001108 from the National Institutes of Health, National Center for Advancing Translational Sciences, Clinical and Translational Sciences Award, and from the Advanced Diagnostics and Therapeutics initiative. We would like to thank Jamie Sanchez, Alexandra Addleton, Lalissie Merga, Elizabeth Peters, Tammy Syed, Mona Arabshahi, and Rick Chappuis for their assistance.

REFERENCES

- Phillips FM, Slosar PJ, Youssef JA, et al. 2013. Lumbar spine fusion for chronic low back pain due to degenerative disc disease: a systematic review. *Spine (Phila Pa 1976)* 38:E409–E422.
- Rajaei SS, Bae HW, Kanim LEA, et al. 2012. Spinal fusion in the United States: analysis of trends from 1998 to 2008. *Spine (Phila Pa 1976)* 37:67–76.
- Deyo RA, Gray DT, Kreuter W, et al. 2005. United States trends in lumbar fusion surgery for degenerative conditions. *Spine (Phila Pa 1976)* 30:1441–1447.
- Fischer CR, Ducoffe AR, Errico TJ. 2014. Posterior lumbar fusion: choice of approach and adjunct techniques. *J Am Acad Orthop Surg* 22:503–511.
- Goldstein CL, Macwan K, Sundararajan K, et al. 2014. Comparative outcomes of minimally invasive surgery for posterior lumbar fusion: a systematic review. *Clin Orthop Relat Res* 472:1727–1737.
- Griffin KS, Davis KM, McKinley TO, et al. 2015. Evolution of bone grafting: bone grafts and tissue engineering strategies for vascularized bone regeneration. *Clin Rev Bone Miner Metab* 13:232–244.
- Benglis D, Wang MY, Levi AD. 2008. A comprehensive review of the safety profile of bone morphogenetic protein in spine surgery. *Neurosurgery* 62:ONS423–ONS431; discussion ONS431.
- Martin BI, Mirza SK, Comstock BA, et al. 2007. Reoperation rates following lumbar spine surgery and the influence of spinal fusion procedures. *Spine (Phila Pa 1976)* 32:382–387.
- Fritsch EW, Heisel J, Rupp S. 1996. The failed back surgery syndrome: reasons, intraoperative findings, and long-term results: a report of 182 operative treatments. *Spine (Phila Pa 1976)* 21:626–633.
- Alanay A, Vyas R, Shamie AN, et al. 2007. Safety and efficacy of implant removal for patients with recurrent back pain after a failed degenerative lumbar spine surgery. *J Spinal Disord Tech* 20:271–277.
- Kornblum MB, Fischgrund JS, Herkowitz HN, et al. 2004. Degenerative lumbar spondylolisthesis with spinal stenosis: a prospective long-term study comparing fusion and pseudarthrosis. *Spine (Phila Pa 1976)* 29:726–734.
- Hu X-Q, Wu X-L, Xu C, et al. 2014. A systematic review and meta-analysis of unilateral versus bilateral pedicle screw fixation in transforaminal lumbar interbody fusion. *PLoS ONE* 9:e87501.
- Hart R, Hermsmeyer JT, Sethi RK, et al. 2015. Quality and quantity of published studies evaluating lumbar fusion during the past 10 years: a systematic review. *Global Spine J* 5:207–218.
- Feiertag MA, Boden SD, Schimandle JH, et al. 1996. A rabbit model for nonunion of lumbar intertransverse process spine arthrodesis. *Spine (Phila Pa 1976)* 21:27–31.
- Rolander SD. 1966. Motion of the lumbar spine with special reference to the stabilizing effect of posterior fusion. An experimental study on autopsy specimens. *Acta Orthop Scand Suppl* 90:1–144.
- Halvorson TL, Kelley LA, Thomas KA, et al. 1994. Effects of bone mineral density on pedicle screw fixation. *Spine (Phila Pa 1976)* 19:2415–2420.
- Korovessis P, Papazisis Z, Koureas G, et al. 2004. Rigid, semirigid versus dynamic instrumentation for degenerative lumbar spinal stenosis. *Spine (Phila Pa 1976)* 29:735–742.
- Boerckel JD, Uhrig BA, Willett NJ, et al. 2011. Mechanical regulation of vascular growth and tissue regeneration in vivo. *Proc Natl Acad Sci USA* 108:E674–E680.
- Brodsky AE, Kovalsky ES, Khalil MA. 1991. Correlation of radiologic assessment of lumbar spine fusions with surgical exploration. *Spine* 16:S261–S265.
- Deckey JE, Court C, Bradford DS. 2000. Loss of sagittal plane correction after removal of spinal implants. *Spine (Phila Pa 1976)* 25:2453–2460.
- Jeon C-H, Lee H-D, Lee Y-S, et al. 2015. Is it beneficial to remove the pedicle screw instrument after successful posterior fusion of thoracolumbar burst fractures? *Spine (Phila Pa 1976)* 40:E627–E633.
- Wild A, Pinto MR, Butler L, et al. 2003. Removal of lumbar instrumentation for the treatment of recurrent low back pain in the absence of pseudarthrosis. *Arch Orthop Trauma Surg* 123:414–418.
- Salerni AA. 2004. Minimally invasive removal or revision of lumbar spinal fixation. *Spine J* 4:701–705.
- Hume M, Capen DA, Nelson RW, et al. 1996. Outcome after Wiltse pedicle screw removal. *J Spinal Disord* 9:121–124.
- Pihlajamäki H, Böstman O, Ruuskanen M, et al. 1996. Posterolateral lumbosacral fusion with transpedicular fixation: 63 consecutive cases followed for 4 (2–6) years. *Acta Orthop Scand* 67:63–68.
- Kuklo TR, Lehman RA. 2003. Effect of various tapping diameters on insertion of thoracic pedicle screws: a biomechanical analysis. *Spine (Phila Pa 1976)* 28:2066–2071.

27. Clements DH, Morledge DE, Martin WH, et al. 1996. Evoked and spontaneous electromyography to evaluate lumbosacral pedicle screw placement. *Spine (Phila Pa 1976)* 21:600–604.
28. Myers BS, Belmont PJ, Richardson WJ, et al. 1996. The role of imaging and in situ biomechanical testing in assessing pedicle screw pull-out strength. *Spine (Phila Pa 1976)* 21:1962–1968.
29. Mackiewicz A, Banach M, Denisiewicz A, et al. 2015. Comparative studies of cervical spine anterior stabilization systems—finite element analysis. *Clin Biomech Elsevier Ltd.* 32:72–79.
30. Whyne CM, Hu SS, Lotz JC. 2001. Parametric finite element analysis of vertebral bodies affected by tumors. *J Biomech* 34:1317–1324.
31. Keaveny TM. 1997. Mechanistic approaches to analysis of trabecular bone. *Forma* 12:267–275.
32. Huiskes R. 1980. Some fundamental aspects of human joint replacement. Analyses of stresses and heat conduction in bone-prosthesis structures. *Acta Orthop Scand Suppl* 185:1–208.
33. Rohlmann A, Zander T, Rao M, et al. 2009. Applying a follower load delivers realistic results for simulating standing. *J Biomech* 42:1520–1526.
34. Rohlmann A, Zander T, Rao M, et al. 2009. Realistic loading conditions for upper body bending. *J Biomech* 42:884–890.
35. Krag MH, Beynon BD, Pope MH, et al. 1986. An internal fixator for posterior application to short segments of the thoracic, lumbar, or lumbosacral spine. Design and testing. *Clin Orthop Relat Res* 203:75–98.
36. Sandén B, Olerud C, Larsson S, et al. 2010. Insertion torque is not a good predictor of pedicle screw loosening after spinal instrumentation: a prospective study in 8 patients. *Patient Saf Surg* 4:14.
37. Zdeblick TA, Kunz DN, Cooke ME, et al. 1993. Pedicle screw pullout strength. Correlation with insertional torque. *Spine* 18:1673–1676.
38. Mehmanparast H, Petit Y, Mac-Thiong J-M. 2015. Comparison of pedicle screw loosening mechanisms and the effect on fixation strength. *J Biomech Eng* 137:121003.
39. Mehmanparast HN, Mac-Thiong JM, Petit Y. 2014. Biomechanical evaluation of pedicle screw loosening mechanism using synthetic bone surrogate of various densities. 36th Annu Int Conf IEEE Eng Med Biol Soc 2014:4346–4349.
40. Helgeson MD, Kang DG, Lehman RA, et al. 2013. Tapping insertional torque allows prediction for better pedicle screw fixation and optimal screw size selection. *Spine J Elsevier Inc.* 13:957–965.
41. Inceoglu S, Ferrara L, McLain RF. 2004. Pedicle screw fixation strength: pullout versus insertional torque. *Spine J* 4:513–518.
42. Oner A, Ely CG, Hermsmeyer JT, et al. 2012. Effectiveness of EMG use in pedicle screw placement for thoracic spinal deformities. *Evid Based Spine Care J* 3:35–43.
43. McAfee PC, Farey ID, Sutterlin CE, et al. 1991. The effect of spinal implant rigidity on vertebral bone-density—a canine model. *Spine (Phila Pa 1976)* 16:S190–S197.
44. Farey I, McAfee P, Gurr K, et al. 1989. Quantitative histologic study of the influence of spinal instrumentation on lumbar fusions: a canine model. *J Orthop Res* 7:709–722.
45. Myers MA, Casciani T, Whitbeck MG, Jr., et al. 1996. Vertebral body osteopenia associated with posterolateral spine fusion in humans. *Spine (Phila Pa 1976)* 21:2368–2371.
46. Boerckel JD, Kolambkar YM, Stevens HY, et al. 2012. Effects of in vivo mechanical loading on large bone defect regeneration. *J Orthop Res* 30:1067–1075.
47. Chen SI, Lin RM, Chang CH. 2003. Biomechanical investigation of pedicle screw-vertebrae complex: a finite element approach using bonded and contact interface conditions. *Med Eng Phys* 25:275–282.
48. Duan Y, Wang HH, Jin AM, et al. 2015. Finite element analysis of posterior cervical fixation. *Orthop Traumatol Surg Res Elsevier Masson SAS* 101:23–29.
49. Bayraktar HH, Morgan EF, Niebur GL, et al. 2004. Comparison of the elastic and yield properties of human femoral trabecular and cortical bone tissue. *J Biomech* 37:27–35.
50. Fradet L, Wang X, Lenke LG, et al. 2016. Biomechanical analysis of proximal junctional failure following adult spinal instrumentation using a comprehensive hybrid modeling approach. *Clin Biomech* 39:122–128.
51. Slyfield CR, Tkachenko EV, Fischer SE, et al. 2012. Mechanical failure begins preferentially near resorption cavities in human vertebral cancellous bone under compression. *Bone* 50:1281–1287.
52. Bianco R-J, Arnoux P-J, Wagnac E, et al. 2017. Minimizing pedicle screw pullout risks: a detailed biomechanical analysis of screw design and placement. *Clin Spine Surg* 30:E226–E232.

SUPPORTING INFORMATION

Additional supporting information may be found in the online version of this article.